

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**

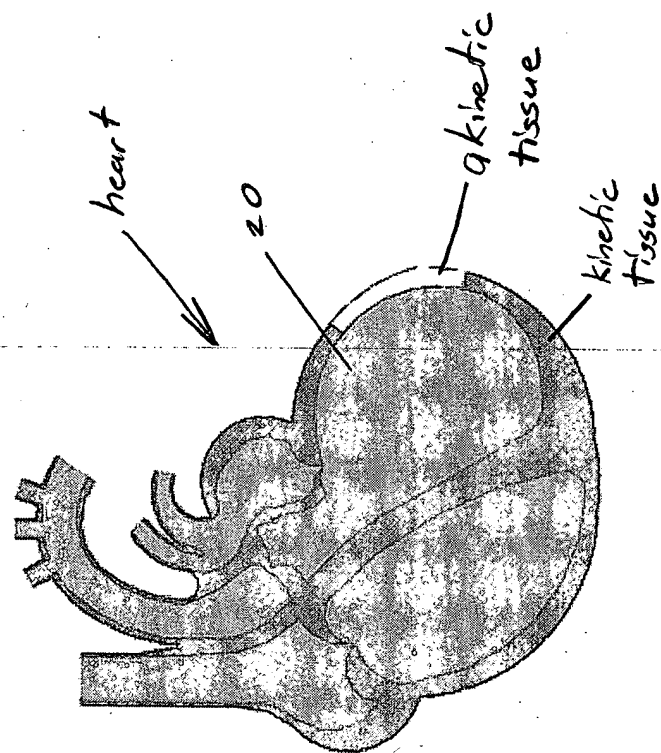


FIG. 1A

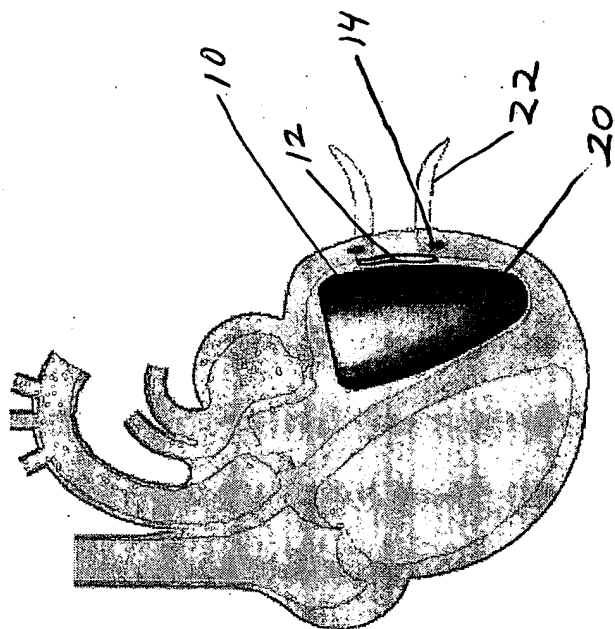


FIG. 1B

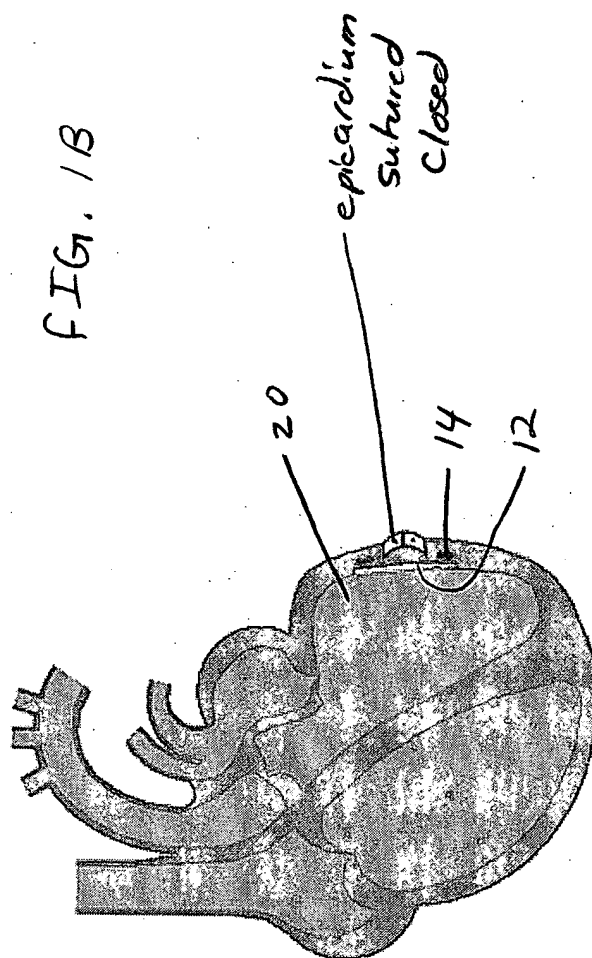


FIG. 1C

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

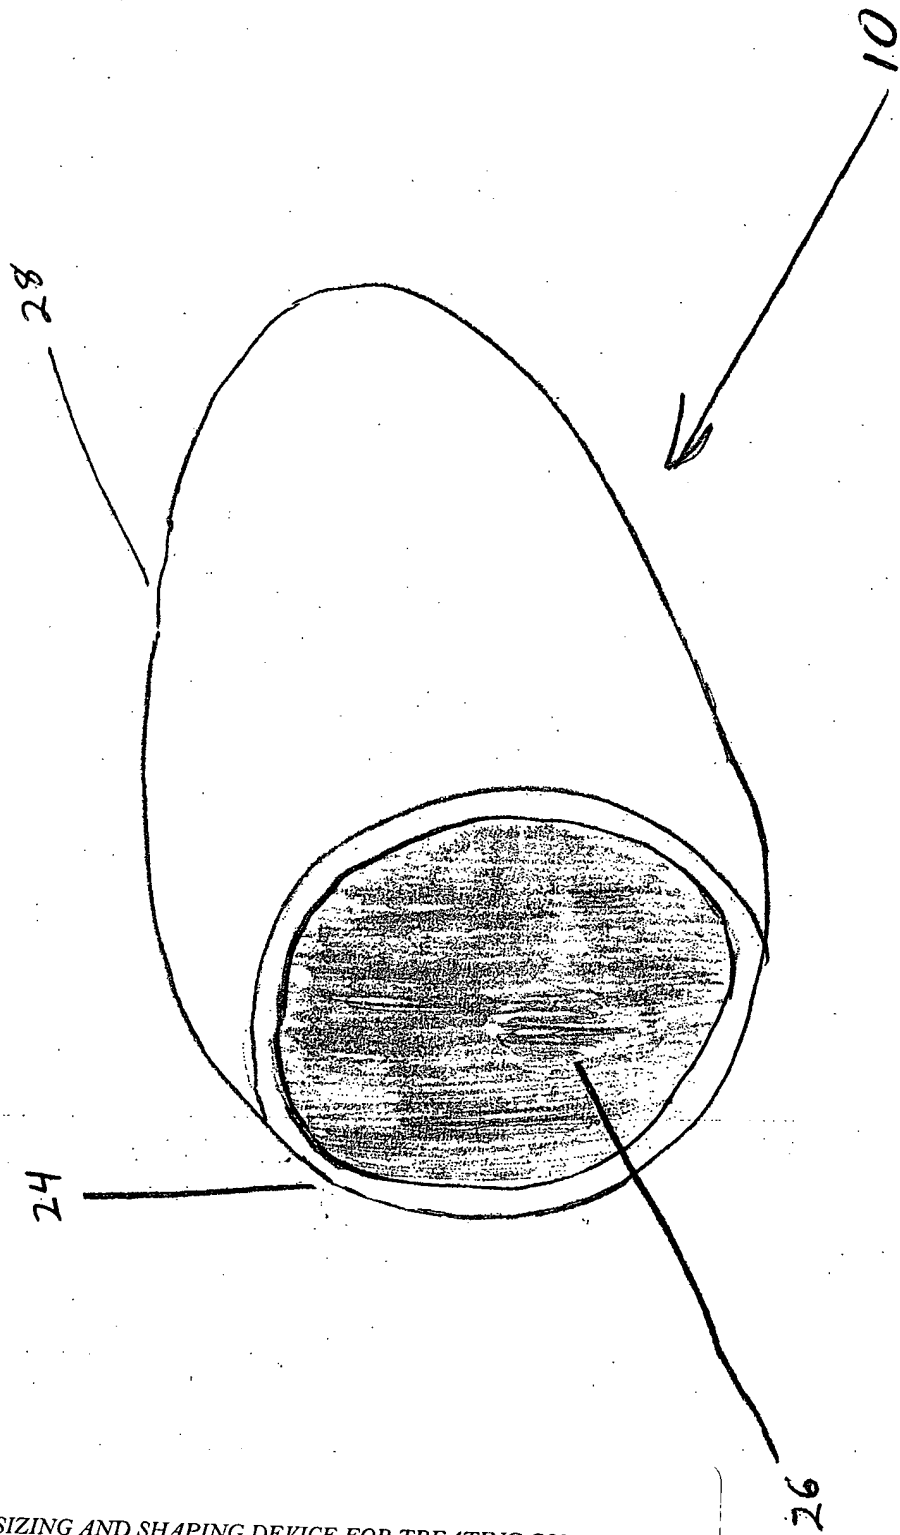


FIG. 2

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

218

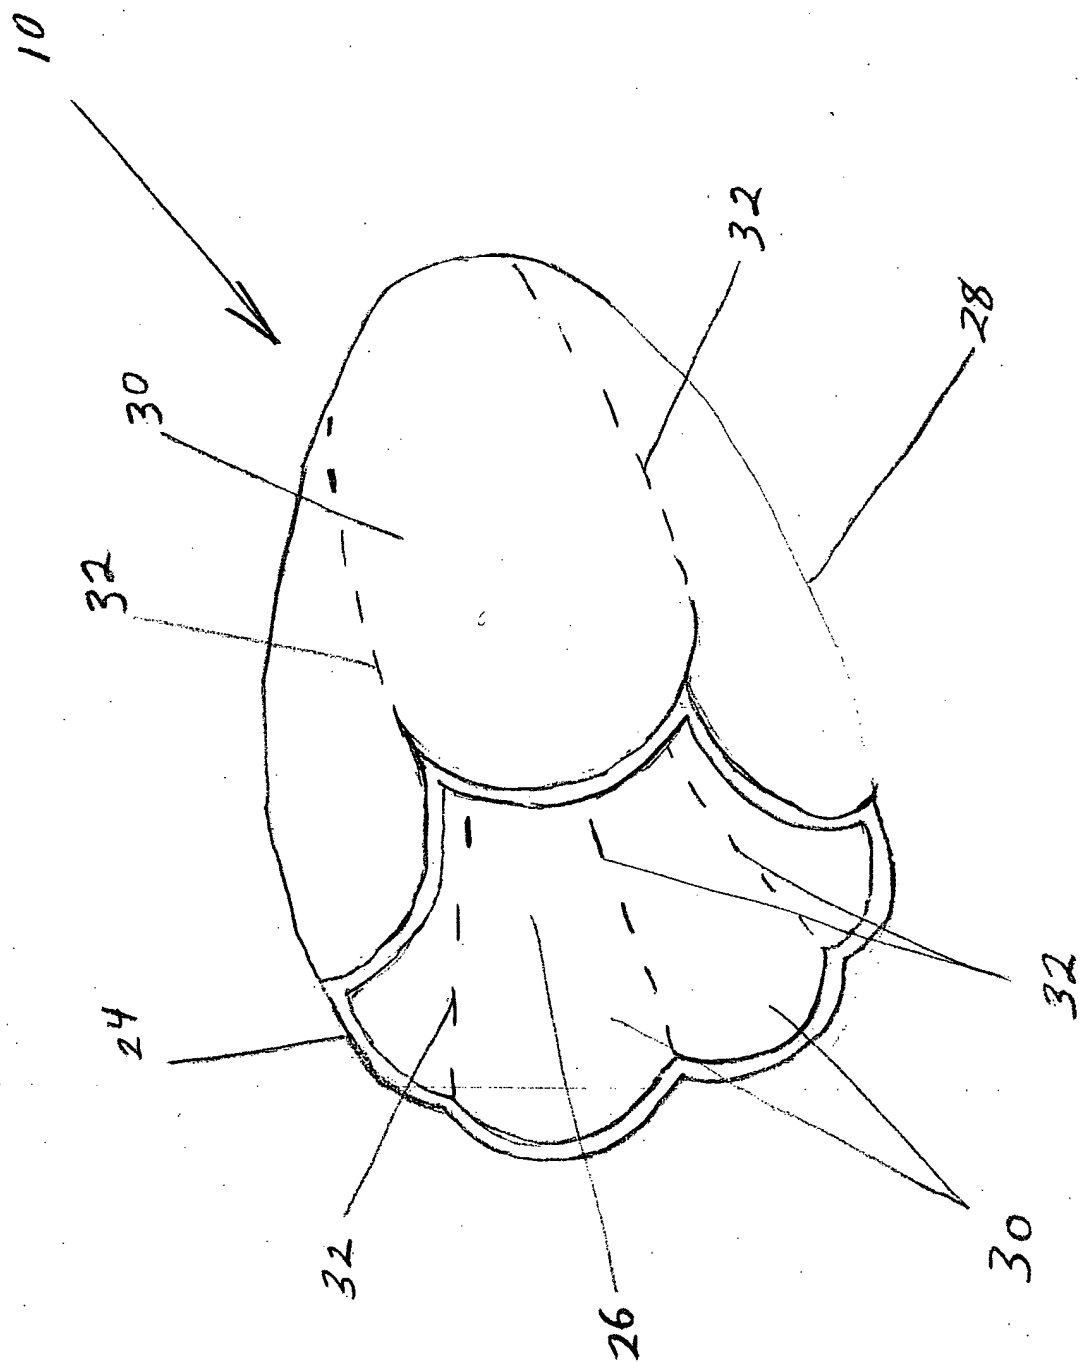


FIG 3

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

3/18.

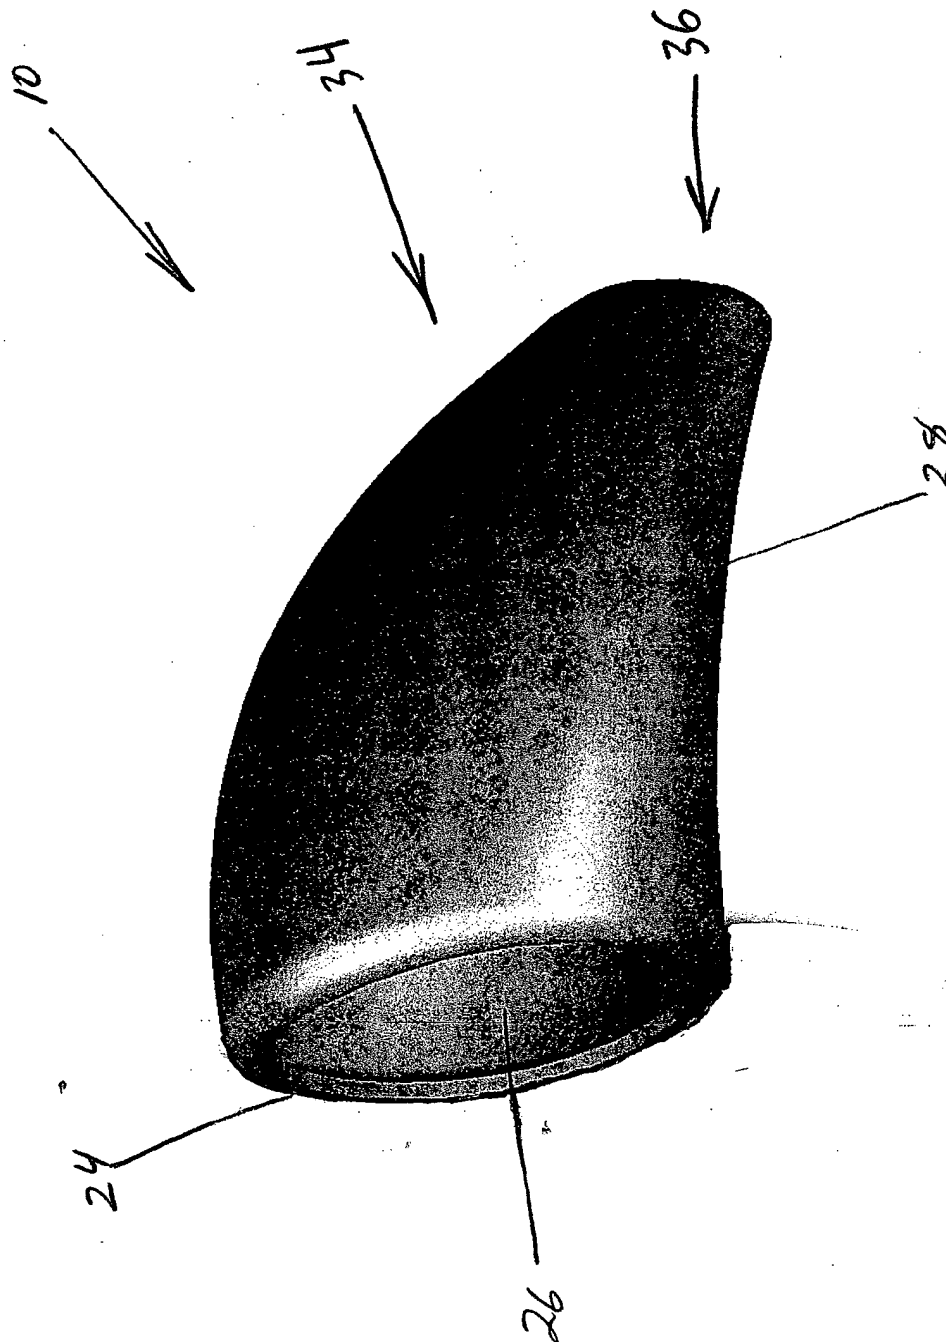


FIG. 4

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

4118

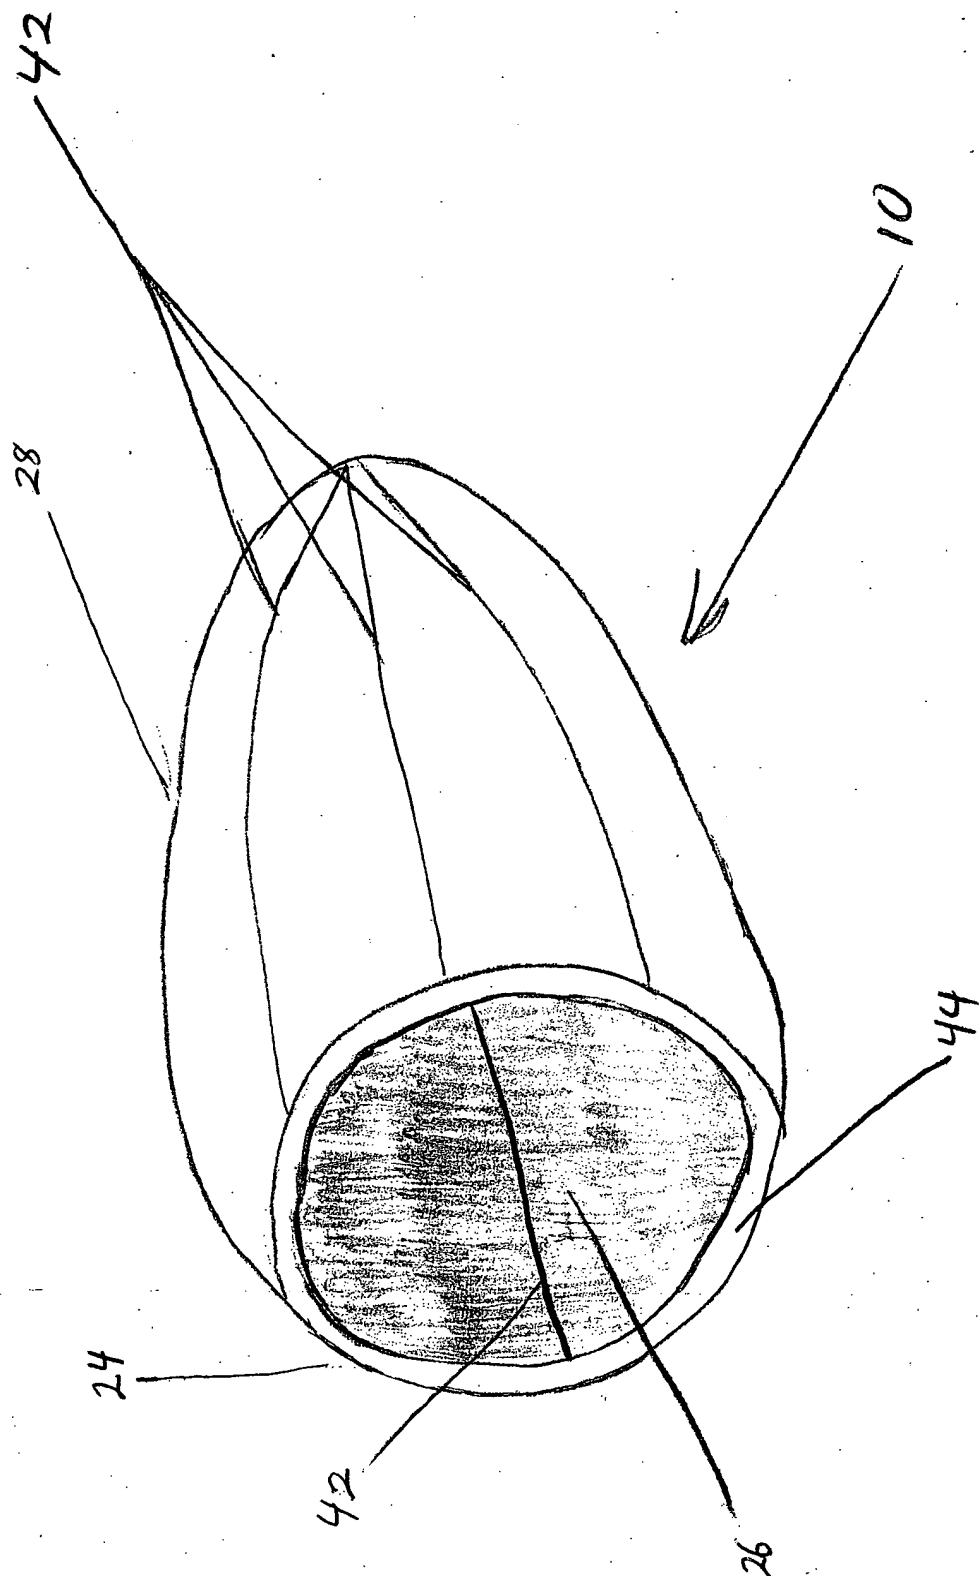


FIG. 5

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

5/18

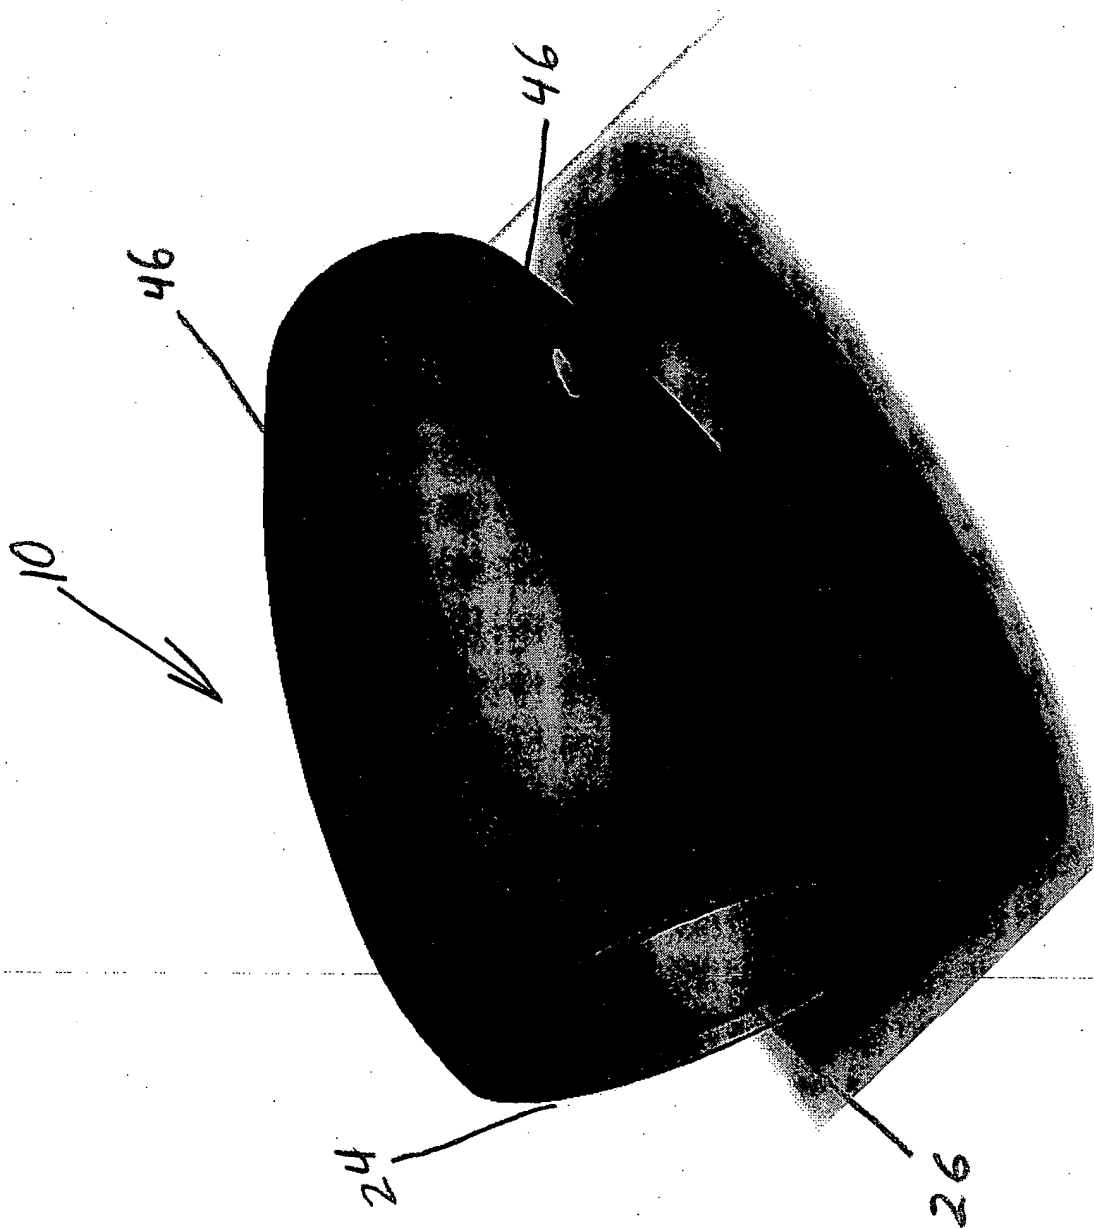


FIG. 6

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

6/18

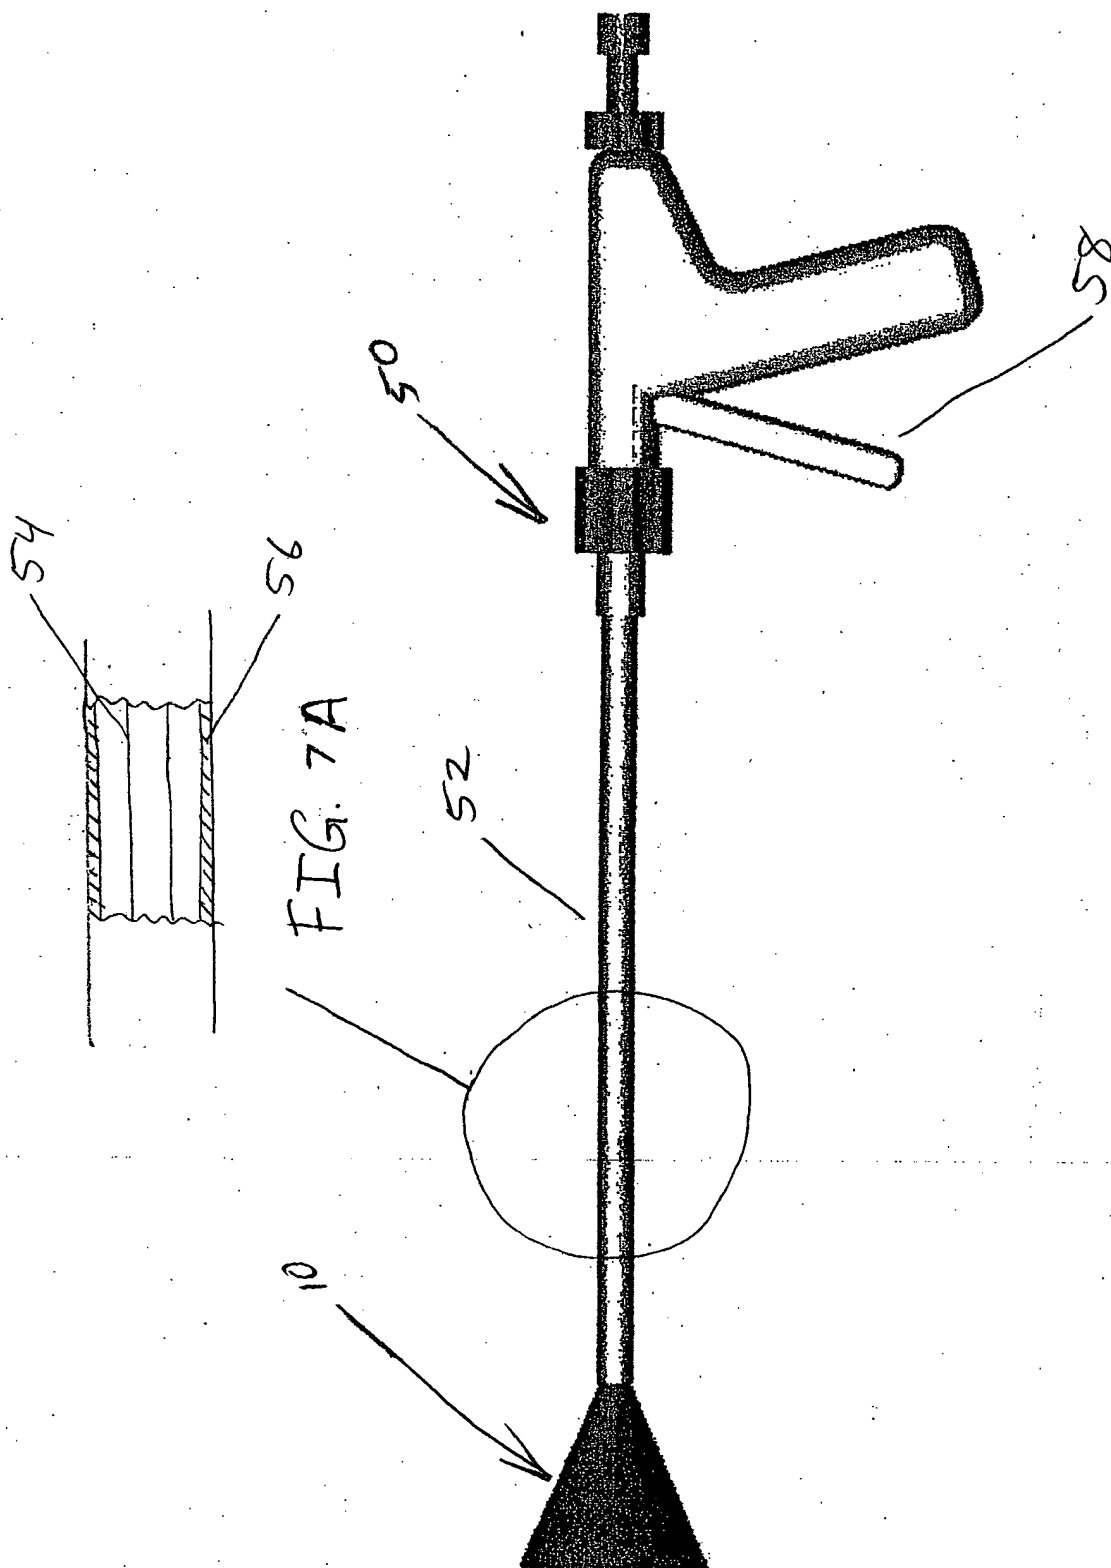


FIG. 7

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown Atty Docket: CHFT.001A

7/18



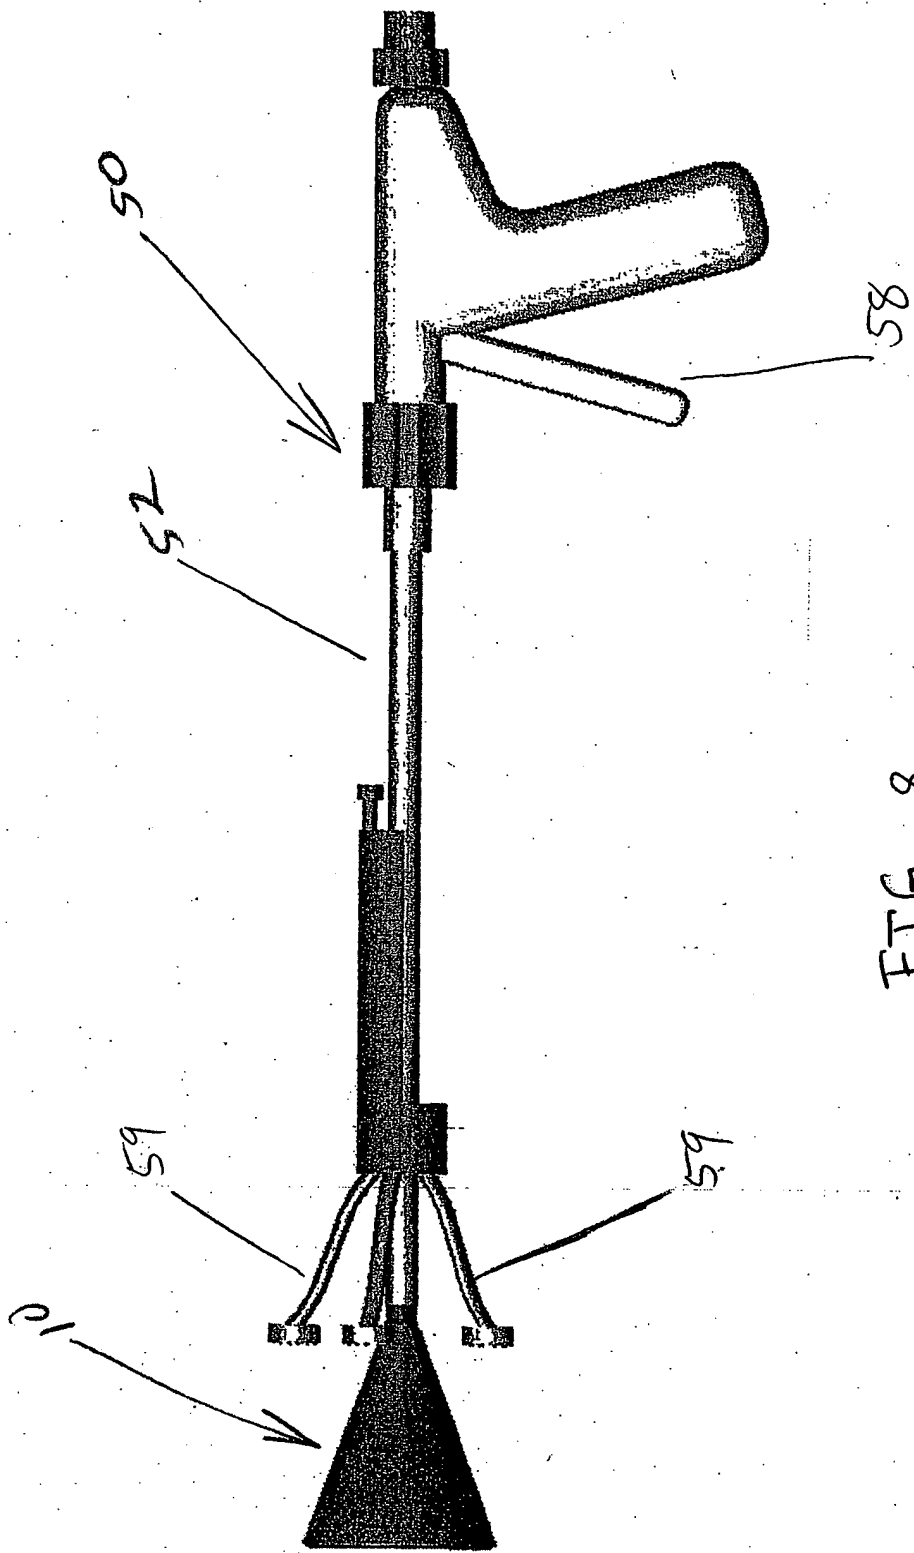


FIG. 8


SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

8/18

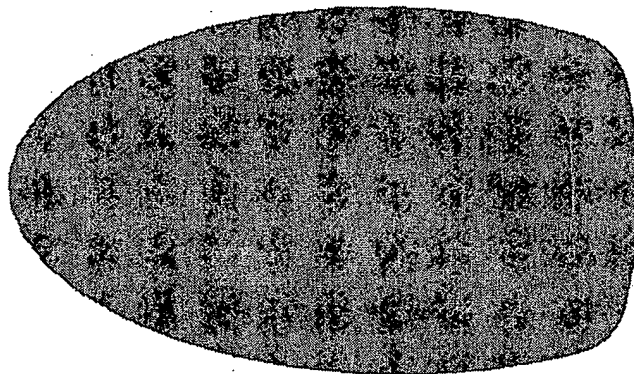

12

FIG. 9

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

9/18

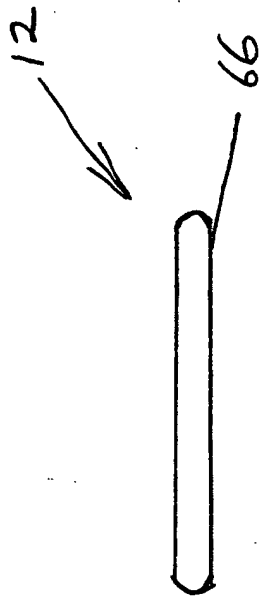


FIG. 11A

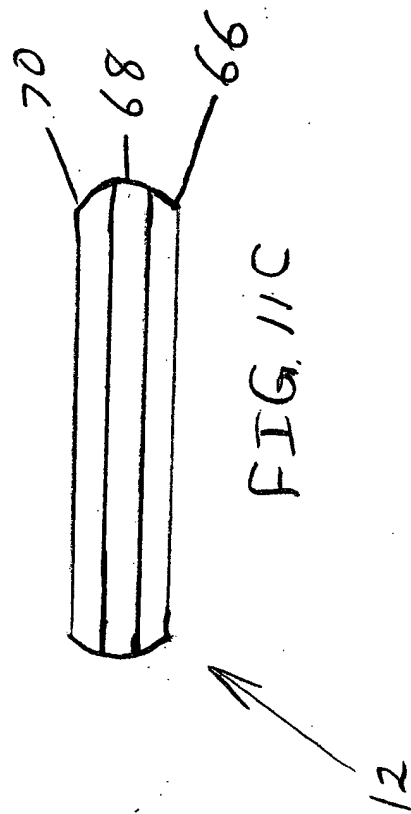


FIG. 11C

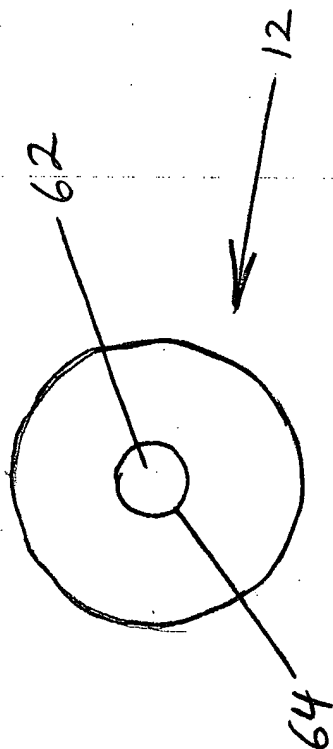


FIG. 10

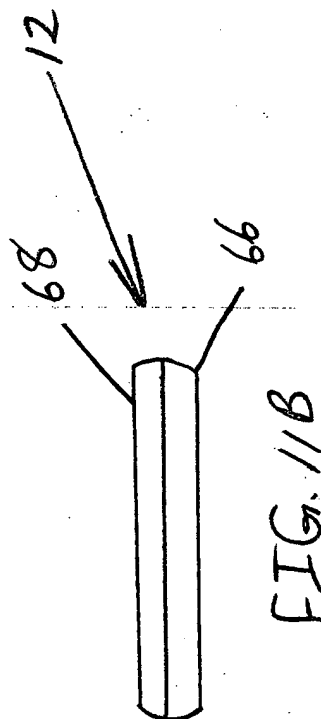


FIG. 11B

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

10/18

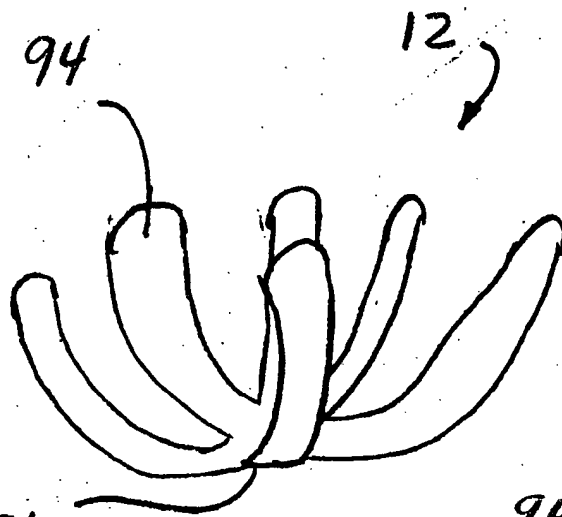


FIG. 12C

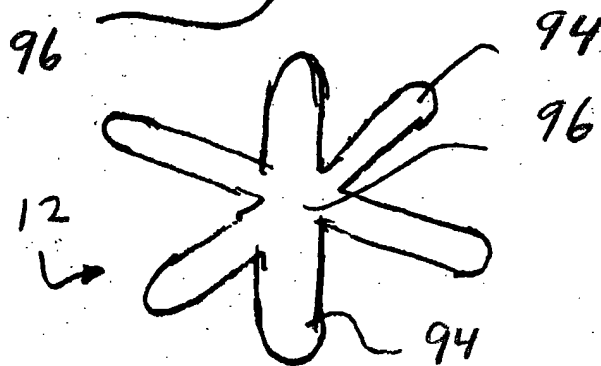


FIG. 12B

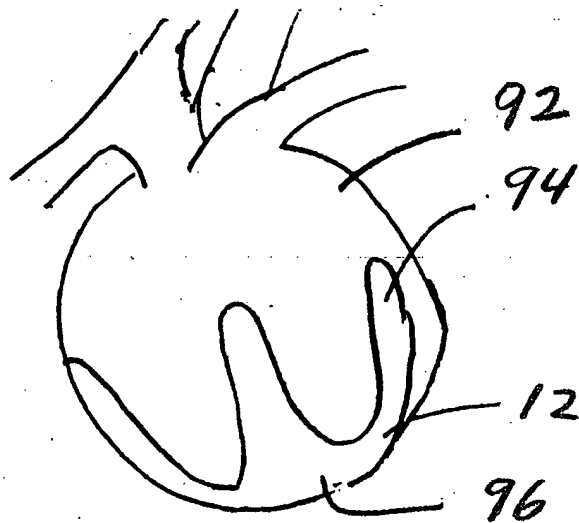


FIG. 12A

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A



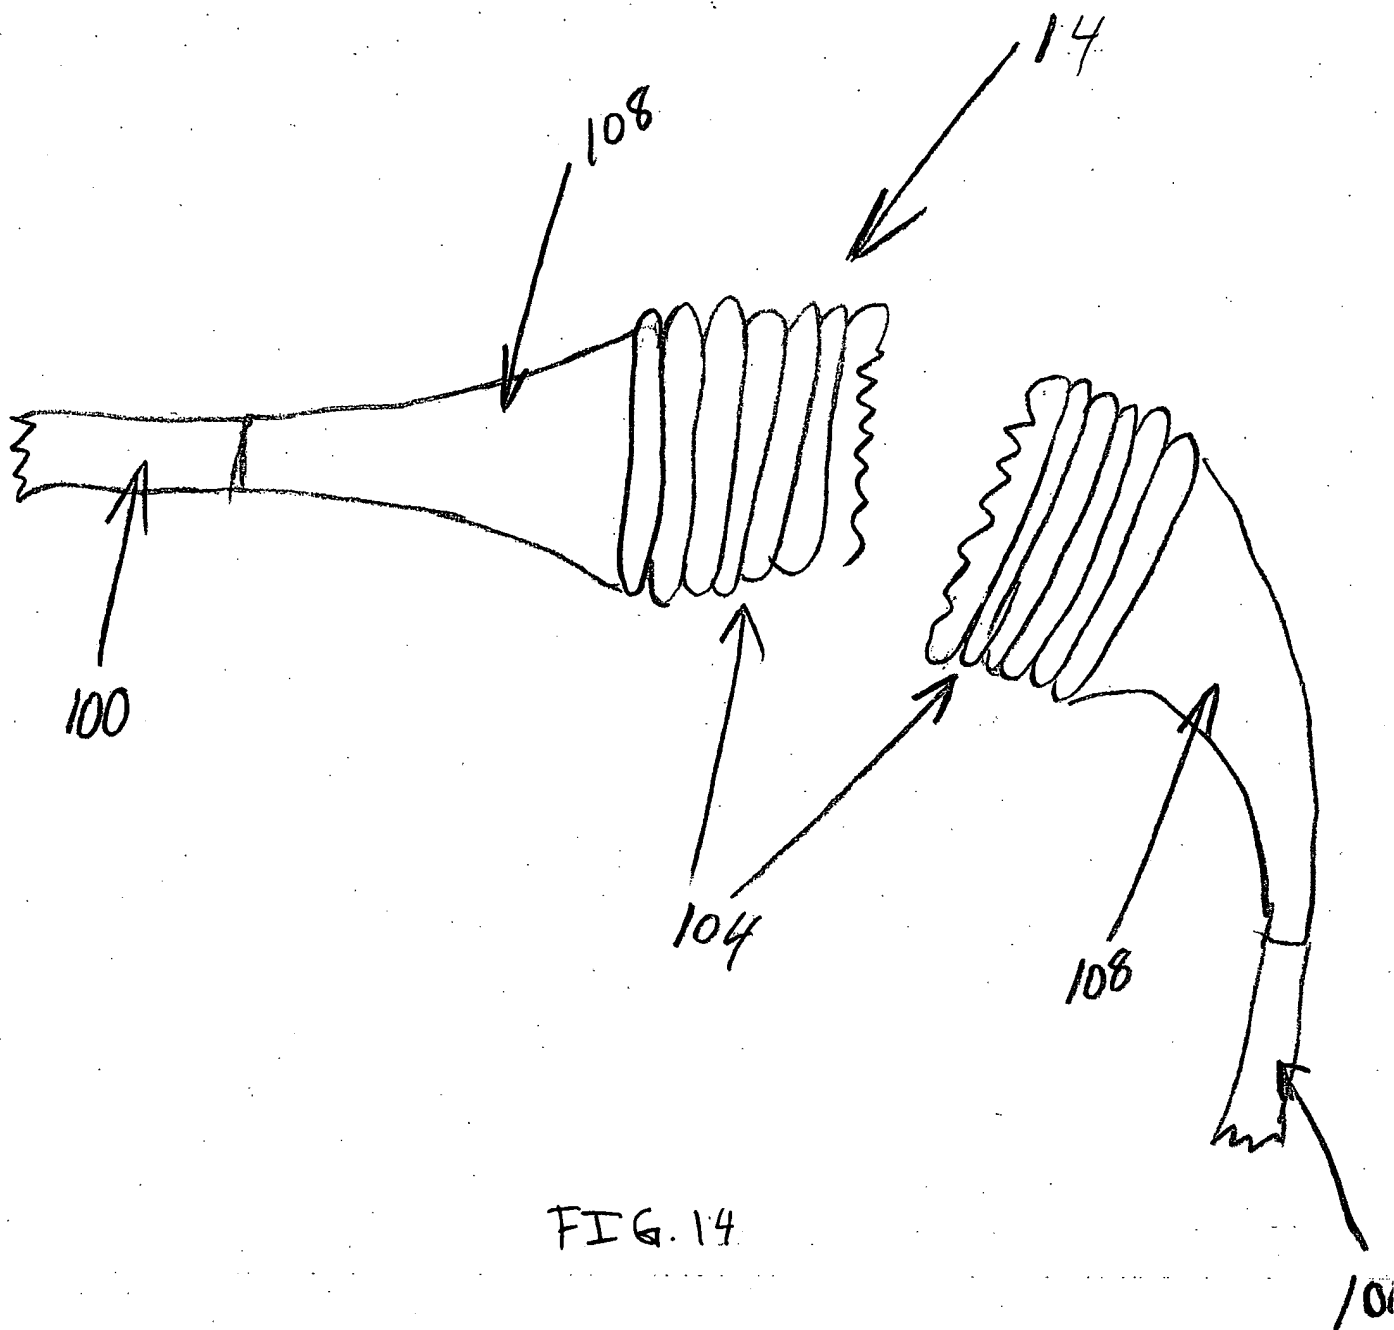


FIG. 14

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

14/18

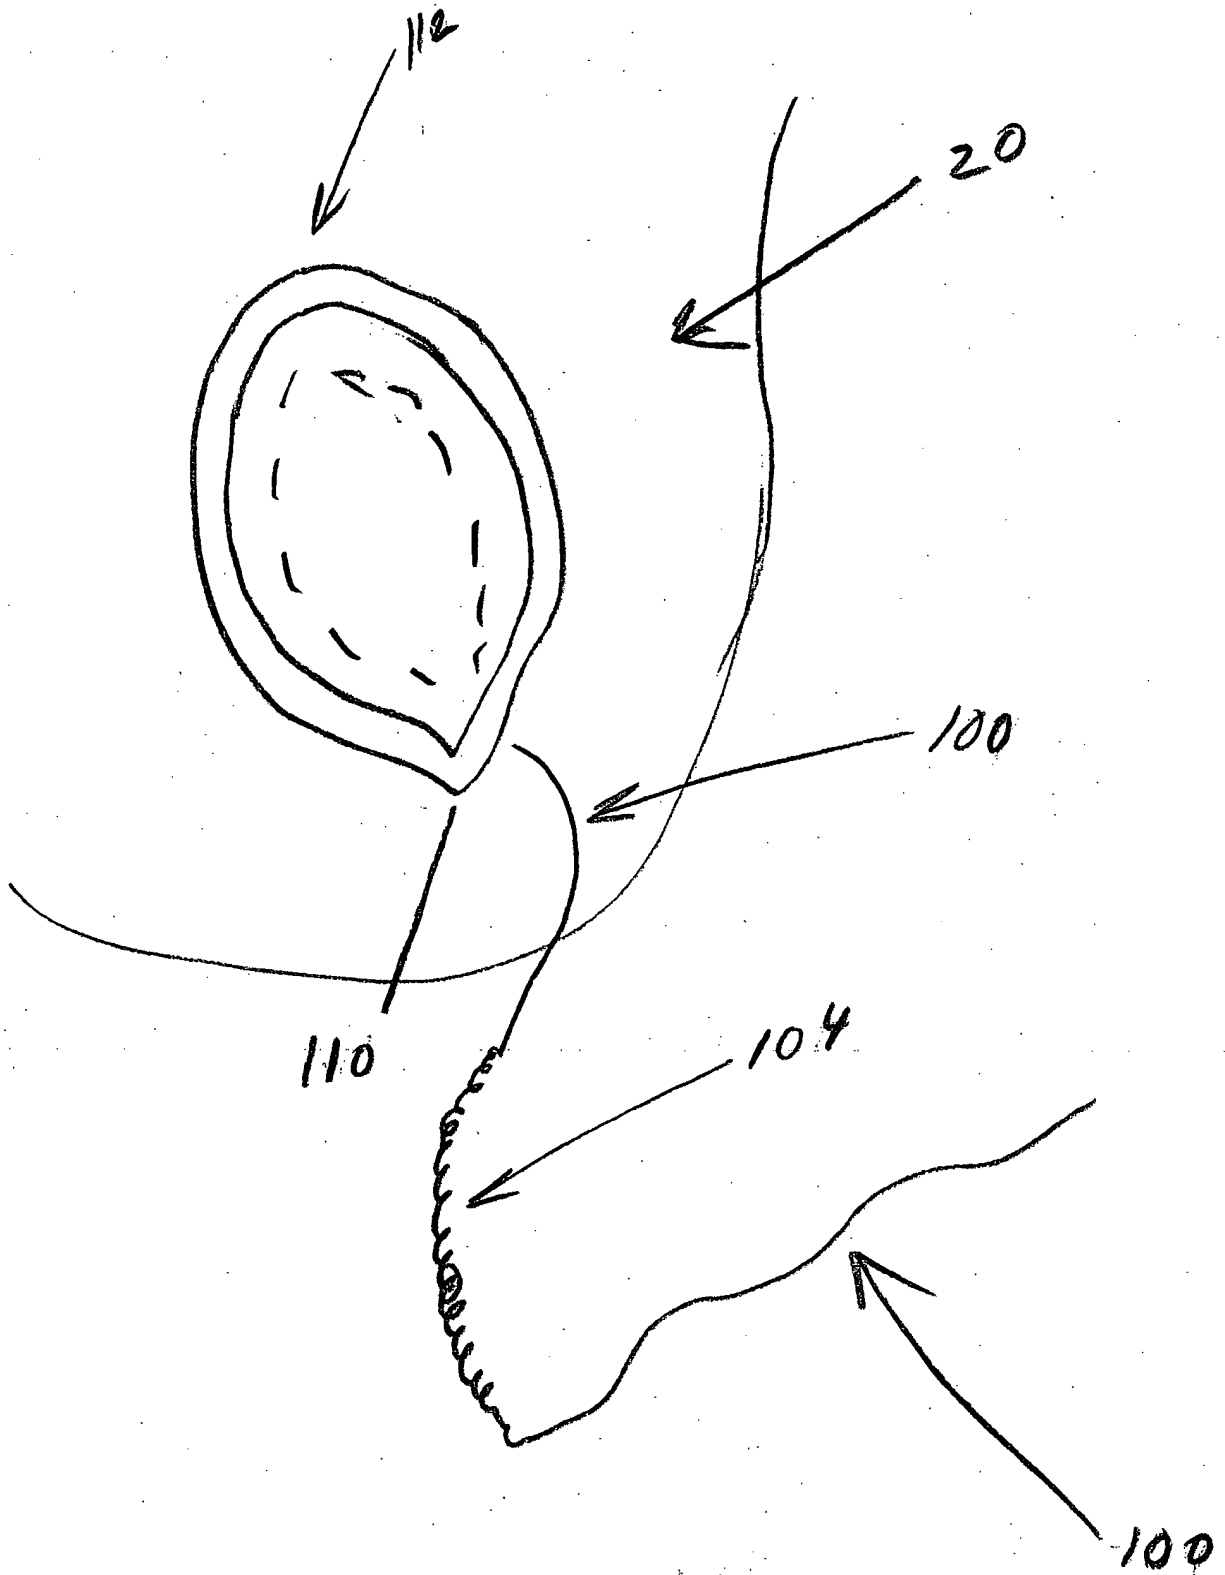


FIG. 15

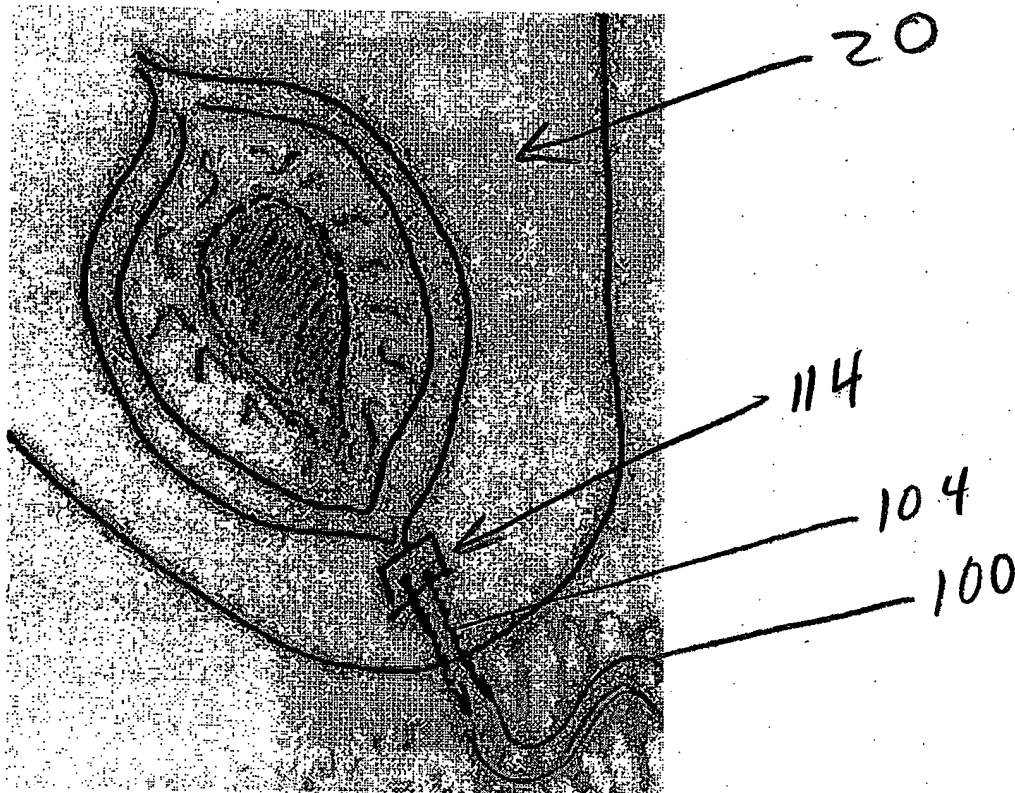


FIG. 16

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

15/18



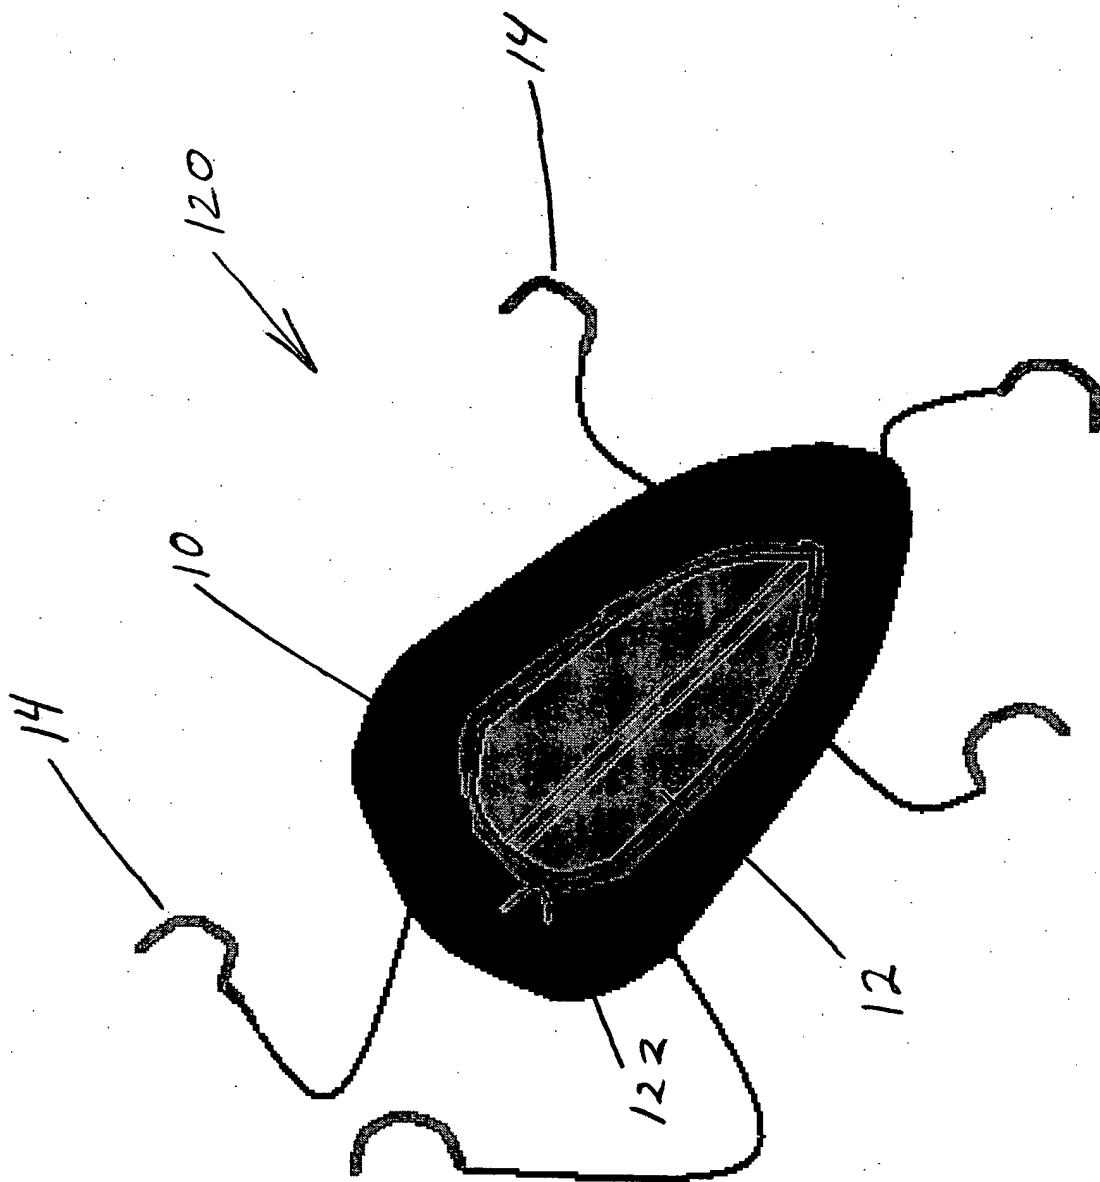


FIG. 17

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

16/18

130

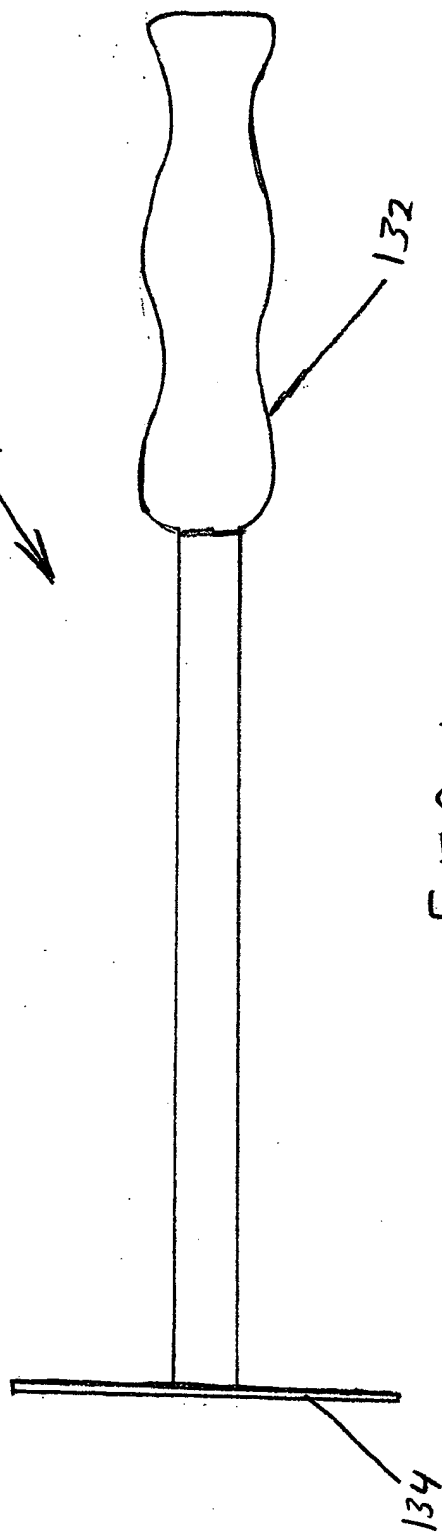


FIG 18

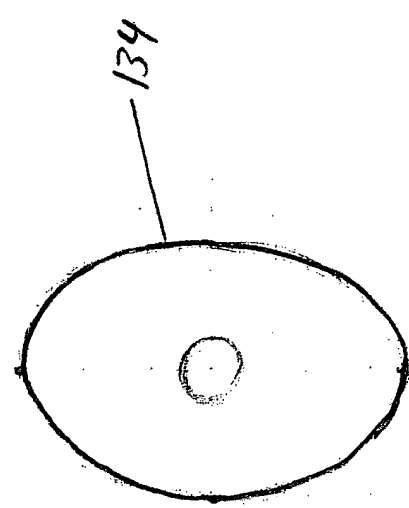



FIG 18A

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown      Atty Docket: CHFT.001A

17/18

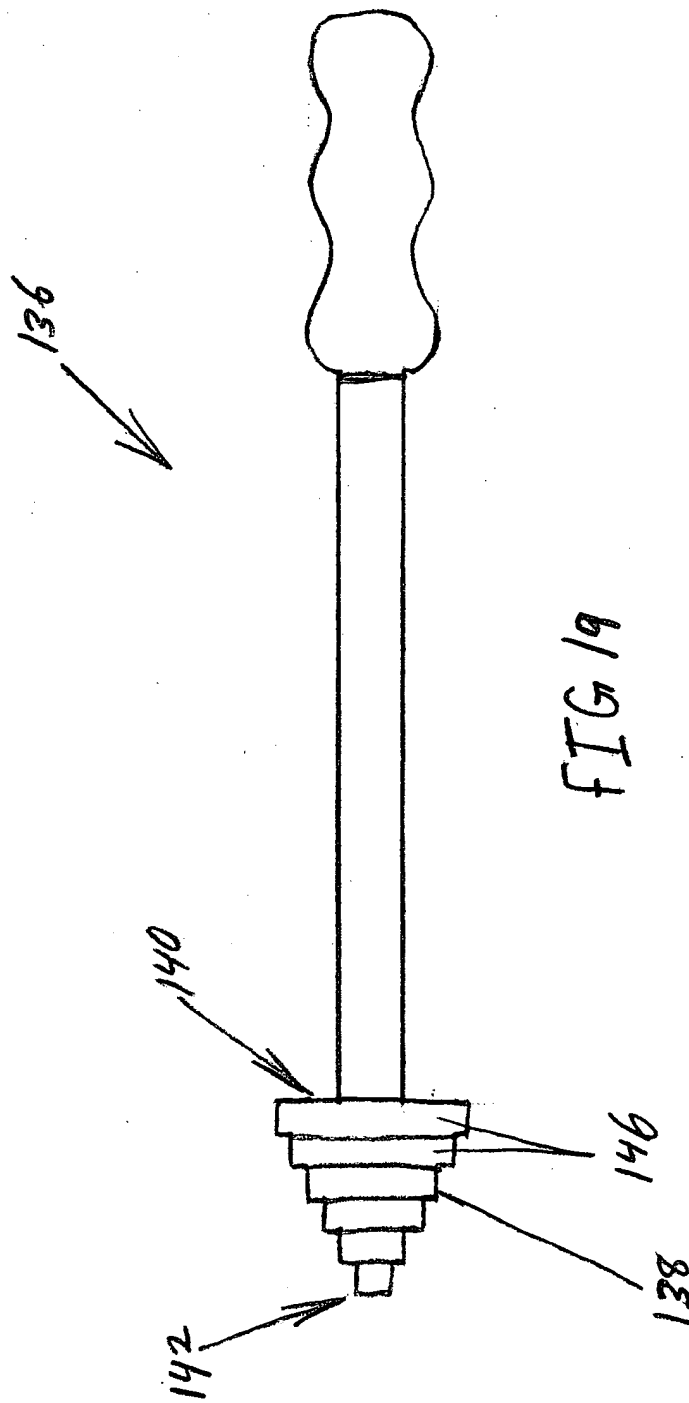

SIZING AND SHAPING DEVICE FOR TREATING CONGESTIVE  
HEART FAILURE

Houser et al.

Appl. No.: Unknown

Atty Docket: CHFT.001A

181